

## 3-IN-1 BLOOD GLUCOSE MONITOR

Step by step





# Contents

---

<b>1 Getting to know your device</b> .....	4
1.1 Included in the delivery and accessories .....	5
1.2 Replacements .....	6
1.3 Functions of the device .....	6
1.4 Signs and symbols .....	7
<b>2 Warnings and safety notes</b> .....	8
<b>3 Description of device and accessories</b> .....	11
3.1 Blood glucose monitor .....	11
3.3 USB cover .....	12
3.4 Display symbols .....	12
3.5 Test strips .....	13
<b>4 Initial use and basic settings</b> .....	14
4.1 Charging the battery .....	14
4.2 Making and changing basic settings .....	15
<b>5 Taking measurements</b> .....	20
5.1 Preparing to take a blood sample .....	20
5.2 Preparing the lancing device for taking a sample .....	21
5.3 Taking a blood sample and measuring the glucose level .....	22
5.4 Reading the result and marking measurements .....	24
5.5 Post-processing and disposal .....	25
5.6 Evaluating measured blood glucose values .....	26
5.7 Functional check using control solution .....	28
<b>6 MEASUREMENT MEMORY</b> .....	30
6.1 Displaying individual values .....	31
6.2 Displaying average blood glucose values for marked values .....	31
6.3 Evaluating measured values on a PC .....	32
<b>7 Storing, maintaining and disinfecting the device</b> .....	32
7.1 Maintenance .....	33
7.2 Disinfection .....	33
<b>8 What if there are problems?</b> .....	34
<b>9 Technical specifications</b> .....	36
<b>10 Comparison of measured values with laboratory values</b> .....	37
<b>11 Usage limits for specialist personnel from the healthcare sector</b> .....	39
<b>12 Warranty/service</b> .....	41

## 1 GETTING TO KNOW YOUR DEVICE

### **Dear customer,**

Thank you for choosing a product from our range. Our name stands for high-quality, thoroughly tested products for applications in the areas of heat, weight, blood pressure, blood glucose, body temperature, pulse, gentle therapy, massage and air.

Please read these instructions for use carefully and keep them for later use. Be sure to make them accessible to other users and observe the information they contain.

With kind regards,  
Your Beurer team.

### **Getting to know your device**

The GL50 evo blood glucose monitor is intended for fast and simple blood glucose measurement of fresh capillary blood samples, either for self-testing or in a clinical environment by trained personnel. It enables you to measure your blood glucose quickly and easily, store the measured values and display the average of all measured values, thereby providing optimum assistance for monitoring your diabetes. The test is performed exclusively externally (IVD).


The backlit display shows measured values clearly. The user-friendly design with handy test strips and the easy operation via a single scroll wheel guarantee simple, yet reliable measurements.

The device can be connected directly to a PC using the integrated USB connection. You can evaluate the measured values on your PC using special software (in English and German language) and use the results to monitor your blood glucose values.

Alternatively, you can transfer the measured values to your smartphone/tablet using the optional Bluetooth® cap.

## 1.1 Included in the delivery and accessories

Check that the set packaging has not been tampered with and make sure that all contents are present. Before use, ensure that there is no visible damage to the device or accessories and that all packaging material has been removed. If you have any doubts, do not use the device and contact your retailer or the specified Customer Service address.

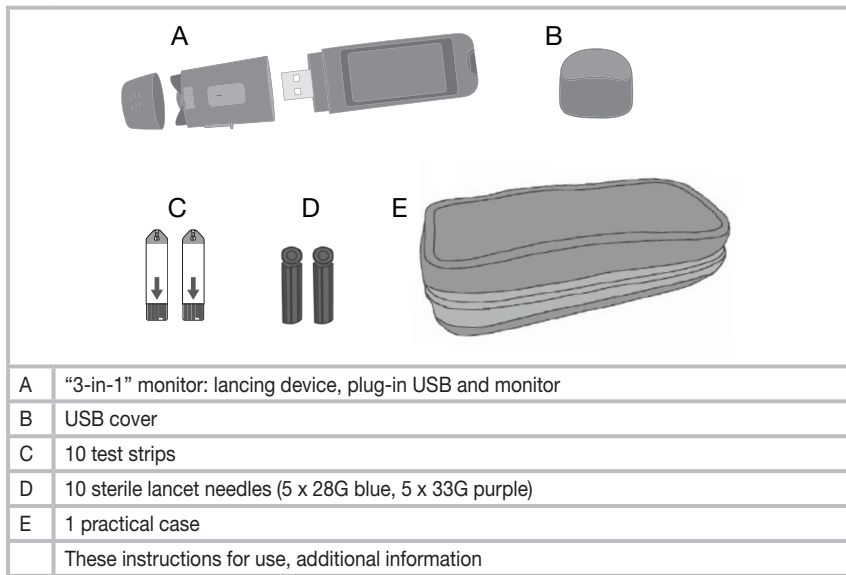

- The blood glucose monitor (A), test strips (C) and additionally available control solutions have been specially designed to complement each other. For this reason, use only test strips (C) and control solutions that have been approved for this blood glucose monitor (A).

### **Note**

- Use original manufacturer accessories only.

## 1.2 Replacements

You can also obtain test strips, control solution and lancets without a prescription.

Item	REF
50 test strips	REF 464.15
50 test strips, individually film packed	REF 464.17
100 test strips	REF 464.13
Control solution LEVEL 3 and 4	REF 464.16
100 soft touch lancets 33G	REF 457.24
100 lancet needles 28G	REF 457.01
100 safety lancets	REF 457.41
200 safety lancets	REF 457.42

## 1.3 Functions of the device

This device is intended for measuring the blood glucose content in human blood. It is also suitable for self-testing at home.

The monitor enables you to quickly and simply:

- Measure your blood glucose level
- Display, mark and save measured values
- Output the measured values acoustically
- Display the average of the measured blood glucose values from the last 7, 14, 30 and 90 days
- Display the average of the marked measured blood glucose values from the last 7, 14, 30 and 90 days
- Set the timer and alarm
- Set the time and date
- Evaluate the saved measured values on a PC using special software
- Transfer the saved measured values to a smartphone/tablet using the optional Bluetooth® cap
- Transfer the saved measured values to a smartphone/tablet using the optional NFC cap

The monitor also includes the following monitoring functions:

- Warning that test strip is insufficiently filled
- Warning in the event of unsuitable temperatures
- Ketone warning
- State of charge display when rechargeable battery is low.























### Warning

- **Do not use the device to diagnose diabetes; it is intended for regular monitoring only**
- **Consult your GP with regard to insulin doses.**

## 1.4 Signs and symbols

The symbols on the packaging and type plate of the monitor and accessories represent the following:

	In vitro diagnostic device
	Serial number
	Temperature limit +2°C to +30°C
	Use by
	Maximum shelf life after initial opening in months
	Batch designation
	Sterilised by radiation (lancets)
	Warning, see accompanying documents
	Medical device (MDR Symbol)
	Rechargeable battery

	Manufacturer
	Observe the instructions for use
	Not for re-use/for single use only
	Green dot (Der Grüne Punkt): German dual waste collection system
	Contents sufficient for <n> tests
	Order number
 	Unit of measurement for blood glucose value
	Biohazard, risk of infection
	<b>CE labelling</b> This product satisfies the requirements of the applicable European and national directives.

In the instructions for use, the symbols represent the following:

 **Warning**

Warning instruction indicating a risk of injury or damage to your health/your patient's health.

 **Important**

Safety note indicating possible damage to the device/accessory.

 **Note**

Note on important information.

## 2 WARNINGS AND SAFETY NOTES

### Risk of infection

All components of the blood glucose monitor and its accessories may come into contact with human blood and are therefore a possible source of infections.



#### Warning

- **Blood glucose values are displayed in mg/dL or mmol/L. You risk damaging your health if you measure your blood glucose value using a unit of measurement with which you are not familiar, misinterpret the values and therefore take incorrect measures. Therefore, please ensure that this monitor displays a unit of measurement with which you are familiar. The unit of measurement accompanies each blood glucose value. Please contact Customer Services if the device displays the incorrect unit of measurement.**
- When using the blood glucose monitor for various persons, observe the generally applicable regulations regarding disinfection, safety and contamination.
- Medical carers and others who use this system on several patients must be aware that all products or objects that come into contact with human blood must be handled, even after cleaning, as though they could transfer pathogens.
- The lancing device is suitable for self-testing. Do not share the lancing device or lancet needles with others or amongst various patients (**risk of infection!**).
- Use a new, sterile lancet needle for each blood sample (**for single use only**).

### General notes



#### Warning

Do not use the device in the vicinity of strong electromagnetic fields and keep it away from radio systems or mobile telephones.

### Measuring the blood glucose content



#### Warning

- The measurements taken by you are for your information only – they are no substitute for a medical examination! Consult your GP regularly regarding your measured values. Never independently alter the procedures prescribed by your GP.
- The Beurer GL50 evo monitor provides a simple way of monitoring your own blood glucose values, however, you may need to obtain information on how to use the system from your healthcare professional (for example, your GP, chemist or diabetes consultant). Only proper use will guarantee exact measurements.
- This device may be used by people with reduced mental capabilities provided that they are supervised or have been instructed on how to use the device safely and are fully aware of the consequent risks of use.
- A lack of water, high fluid loss, for example perspiration, frequent passing of water, severe hypotension (low blood pressure), shock or hyperosmolar hyperglycaemic non-ketotic coma may lead to incorrect measurements.



- A haematocrit value (proportion of red blood cells) between 20% and 60% has no significant influence on the measurement results.
- A very high or low haematocrit value (proportion of red blood cells) may lead to incorrect measurements. In the event of a very high haematocrit value (above 60%), the displayed blood glucose value may be too low; in the event of a very low haematocrit value (below 20%), it may be too high. Consult your GP if you do not know your haematocrit value.
- Do not use the test strips to measure blood glucose values on newborns.
- Do not use NaF or potassium oxalate anticoagulants to prepare for venous blood samples.
- Do not test any severely ill patients using this device.
- Use fresh whole blood only. Do not use serum or plasma.
- Use capillary blood without squeezing the penetration area. Squeezing the area causes the blood to be diluted with tissue fluid and this may lead to an incorrect measurement.
- Do not use the test strips above an altitude of 7010 metres.
- Very high levels of humidity may influence the test results. Relative humidity of more than 90% may lead to inaccurate results.



### Note

The Beurer GL50 evo measuring system is intended for measuring capillary and venous whole blood.

## Storage and maintenance



### Warning

- Store the blood glucose monitor and its accessories out of reach of small children and pets. Small parts, such as lancet needles, cover caps or test strips may be life-threatening when swallowed. If swallowed, seek medical attention immediately.
- The test strip box contains desiccant, which may irritate the skin or eyes when inhaled or swallowed. Keep the box out of the reach of children.

The monitor is made from precision and electronic components. The accuracy of the measured values and service life of the device depend on its careful handling:

- Protect the device and its accessories from impacts, humidity, dirt, marked temperature fluctuations and direct sunlight. Do not store the device, test strips and control solution in your vehicle, in the bathroom or in a cooling appliance.
- Do not drop the device.

## Repairs



### Note

- Do not open the device. Failure to comply with this instruction will void the warranty.
- Do not repair the device yourself. Proper operation can no longer be guaranteed in this case.
- Please contact Customer Services for repairs.

## Disposal



### Warning

- It is essential to comply with the generally applicable safety precautions for handling blood when disposing of materials from the blood glucose monitor. Dispose of all blood samples and materials with which you or your patients come into contact correctly in order to prevent injury and infection of other persons.
- After use, dispose of test strips and lancets in a puncture-proof container.



### Note

Rechargeable batteries must not be disposed of with household waste. As a consumer, you are required by law to recycle used rechargeable batteries. You can recycle your old rechargeable batteries at public collection points in your community or wherever rechargeable batteries of the relevant type are sold.

For environmental reasons, do not dispose of the device in the household waste at the end of its service life. Please dispose of the device in accordance with EC Directive – WEEE (Waste Electrical and Electronic Equipment). If you have any questions, please contact the local authorities responsible for waste disposal.



### Notes on handling batteries

- If your skin or eyes come into contact with fluid from the battery cell, flush out the affected areas with water and seek medical assistance.
- Choking hazard! Small children may swallow and choke on batteries. Store batteries out of the reach of small children.
- If a battery has leaked, put on protective gloves and clean the battery compartment with a dry cloth.
- Risk of explosion! Never throw batteries into a fire.
- Do not disassemble, split or crush the batteries.
- Only use chargers specified in the instructions for use.
- Batteries must be charged correctly prior to use. The instructions from the manufacturer and the specifications in these instructions for use regarding correct charging must be observed at all times.


### Rechargeable battery disposal

- The empty, completely flat rechargeable batteries must be disposed of using specially designated collection boxes, recycling points or electronics retailers. You are legally required to dispose of the batteries.

## 3 DESCRIPTION OF DEVICE AND ACCESSORIES

### 3.1 Blood glucose monitor


#### An overview of the monitor

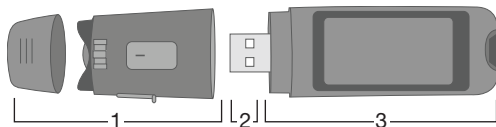

- 1 Lancing device
- 2 Plug-in USB
- 3 Monitor


#### Front

- 1 Display
- 2 Slot for test strips

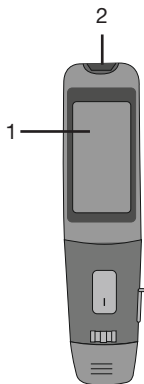


#### Side

- 1 Scroll wheel
- 2 ON/OFF switch
- 3 Tensioning slider




### 3.2 Lancing device and lancet needles

- 1 Cap
- 2 Protective lancet disc
- 3 Sterile lancet needle
- 4 Lancet holder
- 5 Dial for setting different penetration depths
- 6 Tensioning slider
- 7 Trigger

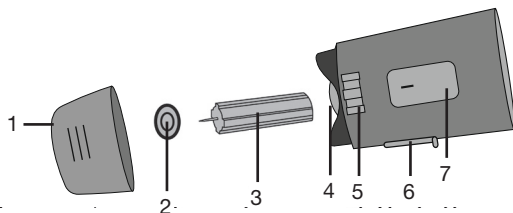


### 3.3 USB cover



If you would like to use the blood glucose monitor without the integrated lancing device, you can use the supplied USB cover in place of the lancing device.

### 3.4 Display symbols

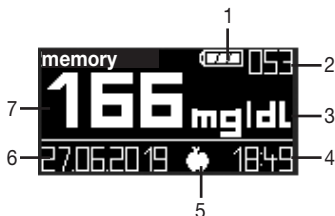

- 1 State of charge
- 2 Memory space number
- 3 Blood sugar unit mg/dL or mmol/L
- 4 Time
- 5 Symbol for marking measurements
- 6 Date
- 7 Measured value display

#### Note

The monitor is supplied with the following basic settings:


- Beep on
- Bluetooth® off
- NFC off
- Ketone warning on
- Language: German

#### Warning

Ensure that you are using the device with the correct blood glucose unit (either mg/dL or mmol/L) setting for you. If in doubt, consult your GP.

## 3.5 Test strips

### Front

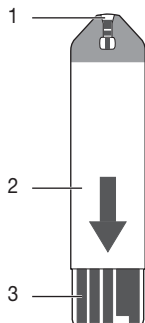


- 1 Gap for blood input
- 2 Grip area
- 3 Contacts

Insert the test strip into the device so that the contacts are pointing inside the slot. Make sure that the front of the test strip is facing you.

### Rear



You can identify the rear by the contact tracks.

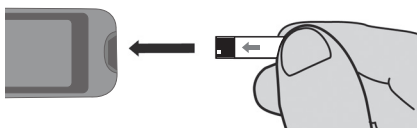

### Note



Read carefully the following information on handling and storing your test strips. The test strips will only provide accurate measurements if all information is followed.


### Warning



Use each test strip only **once** and for **one** patient only!

### Handling test strips

#### Note

- Securely close the test strip box immediately after taking out a test strip.
- Do not use the test strips if they have expired. The use of expired test strips may lead to incorrect measurements. The expiry date is located next to the hourglass symbol  on the box or on the respective film packaging of the individual test strips.
- The test strips expire 18 months after the box is opened (note down the expiry date (date of opening plus 18 months ) on the label. In the event of overlap, the shelf life is limited to the expiry date (see

date next to the hourglass symbol ). This does not apply for individual test strips, which are to be used immediately after opening the film packaging.

- Discontinue use of the test strips if one of the two expiry dates (/ ) has passed.
- You can touch any part of the test strip with clean, dry hands.
- Use the test strip for measurement immediately after removing it from the box/film packaging.
- Do not bend, cut or otherwise modify the test strips.
- Do not use test strips that have come into contact with fluids.

### Storing test strips

#### Note

- Keep the test strips in a cool, dry place above +2°C and below +30°C. Do not expose the test strips to direct sunlight or heat. Do not store in your vehicle, in the bathroom or in a cooling appliance.
- Permitted relative air humidity below 90%.
- The test strips must be stored in the original box/unopened film packaging – never use other containers.

## 4 INITIAL USE AND BASIC SETTINGS

In order to activate the device, move the ON/OFF switch into the “ON” position.



The ON/OFF switch is used as a keylock for the scroll wheel.

#### Information regarding initial use

- Before putting the blood glucose monitor into operation for the first time, you must fully charge the rechargeable battery. To charge the rechargeable battery, proceed as directed in the following chapter.
- Before the initial use, no battery symbol will be displayed during charging.

### 4.1 Charging the battery

- 1 Remove the lancing device from the blood glucose monitor.
- 2 Connect the blood glucose monitor to a computer via the USB port.  
Leave the blood glucose monitor to charge for at least 2 hours.
- 3 Once you have fully charged the rechargeable battery of the blood glucose monitor, disconnect the blood glucose monitor from the computer.
- 4 Place the lancing device back on the blood glucose monitor.  
After charging the battery, wait 30 minutes before carrying out a blood glucose measurement.

## 4.2 Making and changing basic settings

### 1 Setting the date and time


#### Note

You must set the date and time. Otherwise, you will not be able to save your measured values correctly with a date and time and access them again later.


The time can be displayed in 12-hour format or 24-hour format.

1. Switch on the blood glucose monitor by briefly pressing and holding the scroll wheel.


2. Rotate the scroll wheel until the arrow is pointing towards “Settings”, then press the scroll wheel.



3. Rotate the scroll wheel until the arrow is pointing towards “Date/time”, then press the scroll wheel.




4. Set the year by rotating the scroll wheel, then press the scroll wheel.



5. Use the same procedure to set the month, day, 24 h or 12 h mode, hour and minute.



6. To save the settings, rotate the scroll wheel until the arrow is pointing towards “Save” and confirm by pressing the scroll wheel.



## 2 Setting the timer

You can set a timer on the blood glucose monitor. A beep sounds when the timer elapses. To set a timer, proceed as follows:




1. Switch on the blood glucose monitor by briefly pressing and holding the scroll wheel.
2. Rotate the scroll wheel until the arrow is pointing towards "Settings", then press the scroll wheel to confirm.
3. Rotate the scroll wheel until the arrow is pointing towards "Timer", then press the scroll wheel.
4. Rotate the scroll wheel until the hour is marked, then press the scroll wheel. Now set your desired timer hour by rotating the scroll wheel and press the scroll wheel to confirm.
5. Use the same procedure to set the timer minute.
6. In order to start the timer, rotate the scroll wheel to "Start" and press the scroll wheel.



## 3 Setting the alarm

You can set an alarm on the blood glucose monitor. A beep sounds at the set alarm time. You can set 4 different alarm times. To set an alarm, proceed as follows:

1. Switch on the blood glucose monitor by briefly pressing and holding the scroll wheel.
2. Rotate the scroll wheel until the arrow is pointing towards "Settings", then press the scroll wheel to confirm.
3. Rotate the scroll wheel until the arrow is pointing towards "Alarm", then press the scroll wheel.
4. Select one of the 4 alarm times with the scroll wheel and press the scroll wheel.
5. Now set your desired alarm hour by rotating the scroll wheel and press the scroll wheel to confirm. Use the same procedure to set the alarm minute.








- 3
6. In order to start the alarm, rotate the scroll wheel to “On” and press the scroll wheel.
  7. In order to turn off the alarm, rotate the scroll wheel to “Off” and press the scroll wheel.



4 **Switching Bluetooth® or NFC on/off**

You can switch on Bluetooth®/NFC on the blood glucose monitor.

1. Switch on the blood glucose monitor by briefly pressing and holding the scroll wheel.
2. Rotate the scroll wheel until the arrow is pointing towards “Settings”, then press the scroll wheel.
3. Rotate the scroll wheel until the arrow is pointing towards “Bluetooth on/off” or “NFC on/off” and press the scroll wheel.
4. Rotate the scroll wheel until the arrow is pointing towards “Bluetooth on”, then press the scroll wheel. Bluetooth® is now switched on. Proceed in the same manner to switch on NFC.




## 5 **Switching the beep on/off**


On the blood glucose monitor, you can switch on the beep, switch off the beep or set a result beep.

1. Switch on the blood glucose monitor by briefly pressing and holding the scroll wheel.


2. Rotate the scroll wheel until the arrow is pointing towards “Settings”, then press the scroll wheel.



3. Rotate the scroll wheel until the arrow is pointing towards “Beep on/off”, then press the scroll wheel.



4. Use the scroll wheel to select your desired setting (beep on, beep off or result beep) and confirm by pressing the scroll wheel.



### **Note**

The result beep transmits the measurement as an acoustic beep signal.

Example: measured value 103




The beep signal is repeated 2 times and can be interrupted by rotating the scroll wheel.

## 6 **Switching the ketone warning on/off**


On the blood glucose monitor, you can switch a ketone warning on and off.

1. Switch on the blood glucose monitor by briefly pressing and holding the scroll wheel.


2. Rotate the scroll wheel until the arrow is pointing towards “Settings”, then press the scroll wheel.



3. Rotate the scroll wheel until the arrow is pointing towards “Ketone on/off”, then press the scroll wheel.



- 6 4. Use the scroll wheel to select your desired setting (warning on or warning off) and confirm by pressing the scroll wheel.




• Ketone  
• Warning on ✓  
• Warning off  
↶ Back

## 7 Turning the display


You can turn the display on the blood glucose monitor.

1. Switch on the blood glucose monitor by briefly pressing and holding the scroll wheel.
2. Rotate the scroll wheel until the arrow is pointing towards “Settings”, then press the scroll wheel.



• All values  
• Average  
• Settings ←  
↶ Back

3. Rotate the scroll wheel until the arrow is pointing towards “Turn display”, then press the scroll wheel.




• Beep on/off  
• Ketone on/off  
• Turn display ←  
• Language

## 8 Selecting the menu language


The following menu languages are available: English, German, French, Spanish, Italian and Turkish.

1. Switch on the blood glucose monitor by briefly pressing and holding the scroll wheel.
2. Rotate the scroll wheel until the arrow is pointing towards “Settings”, then press the scroll wheel.



• All values  
• Average  
• Settings ←  
↶ Back

3. Rotate the scroll wheel until the arrow is pointing towards “Language”, then press the scroll wheel.



• Ketone on/off  
• Turn display  
• Language ←  
↶ Back

4. Use the scroll wheel to select your desired menu language and confirm by pressing the scroll wheel.



• Language  
• 🇩🇪 Deutsch ✓ ←  
• 🇬🇧 English  
• 🇫🇷 Français ▼

## 5 TAKING MEASUREMENTS



### Warning

- If the protective disc on a lancet needle has already been removed, do not use the lancet needle.
- If you drop the lancing device with an inserted lancet needle, carefully pick it up and dispose of the lancet.



### Important

- Use the lancing device only with lancet needles from the same manufacturer. Using other lancet needles may prevent the lancing device from working properly.
- If you are using a third-party lancing device, please read the accompanying instructions for use.

### 5.1 Preparing to take a blood sample

#### 1 Choose a part of the body from which to take a blood sample

Using the lancing device, you can take a blood sample from the fingertip. To make the procedure as painless as possible, do not take samples directly from the centre of the fingertip, but slightly to either side.




### Warning

- **In the event of suspected hypoglycaemia: take blood from the fingertip only.** Reason: changes to blood glucose levels can be detected quickly in blood samples taken from the fingertip.

#### 2 Prepare all parts

Prepare the following items: GL50 evo measuring device (A), test strip box or test strips in film packaging (C) and sterile lancet needles (D).

Make sure that the ON/OFF switch is in the "ON" position. 

#### 3 Wash your hands

Wash your hands with soap and warm water before taking a blood sample. This not only ensures optimal hygiene but also encourages good blood circulation at the puncture area on the finger. Dry your hands carefully.




### Warning

If you have used alcohol for cleaning, ensure that the area has fully dried prior to measuring.

## 5.2 Preparing the lancing device for taking a sample


### 1 Remove the cap

Securely hold the monitor with one hand on the lancing device cover. With your other hand, remove the cap from the monitor's lancing device.




### 2 Insert the lancet needle

Insert a sterile lancet needle into the lancing device.



#### Note


Your starter set contains lancet needles in 2 different sizes. If you are unable to take an adequate blood sample using the smaller needles (purple, 33G), please use the slightly larger needles (blue, 28G).




Push firmly on the lancet until it audibly engages and it cannot be pushed further into the holder.

### 3 Remove the protective lancet disc

Remove the protective lancet disc by bringing it into a horizontal position and taking it off. Retain the protective disc for the safe disposal of the used lancet needle after taking a blood sample.



4 Place the cap onto the lancing device. Make sure that the curved part of the cap fits on the curved part of the lancing device. Press firmly on the cap until it audibly engages.



### 5 Select the penetration depth

You can set seven different penetration depths on the lancing device using the dial with printed numbers.


- 1 to 2: soft or thin skin
- 3 to 5: normal skin
- 6 to 7: thick or calloused skin

Turn the dial until the required bar is in the centre of the black marking.



### 6 Tension the lancing device

Pull back the slider in the direction of the arrow (on the image: to the right) until it stops and then release. The slider automatically springs back into position. The lancing device is now tensioned.



### 5.3 Taking a blood sample and measuring the glucose level



#### Warning

- Change the puncture area each time you take a measurement, e.g. use a different finger or the other hand. Repeatedly using the same area may cause inflammation or scarring.
- If the cap is not in place, there is a risk of injury from the exposed lancet.
- Do not squeeze your finger to obtain a larger drop of blood. If squeezed, the blood is diluted with tissue fluid and this may lead to an incorrect measurement.
- Please note that insufficient blood circulation at the puncture area, e.g. caused by cold temperatures or illness, can lead to incorrect results.



#### Important

Do not apply any blood samples or control solutions to the test strip before inserting it in the monitor.


#### 1 Prepare the test strip

Take a test strip from the box/film packaging and immediately close it again. Use the test strip within three minutes of removal.

#### 2 Insert test strip

Take the monitor in your left hand. Hold the monitor so that the display is facing you.

Insert the test strip into the slot on the rear end of the blood glucose monitor with the contacts first. Make sure that the front of the test strip is facing you. You can touch any part of the test strip with clean, dry hands.



#### 3 The device switches on automatically

After you have inserted the test strip, the blood glucose monitor switches on automatically and the Beurer logo, the date and the time are briefly displayed. The measuring device is ready to measure as soon as the test strip animation is displayed.



#### Important


If segments of the display are missing, stop using the device and immediately contact Customer Services.

#### 4 Lancing to take a blood sample

The lancing device can now be used to take a blood sample. Make sure that the blood remains as a droplet and is not spread.

##### Blood sample from the fingertip

Firmly position the lancing device slightly to the side of the centre of the fingertip. Press the trigger. Remove the lancing device from the finger. A round drop of blood of at least 0.6 microlitres (corresponds to approx. 1.4 mm in diameter, original size: ●) must have formed.



##### Please also note the following:

- If the blood glucose test results do not match how you feel, carry out another test using blood from your fingertip.
- DO NOT change your treatment purely on the basis of a measurement that was carried out using blood taken from an alternative area. Carry out another test with blood from your fingertip in order to confirm the test result.
- If you often fail to notice that you have a low blood glucose level, carry out a test using blood from your fingertip.


#### 5 If necessary, repeat the lancing process

If you do not obtain sufficient blood, repeat the lancing process with a greater penetration depth in a different area.

#### 6 Apply blood to the test strip

Turn the monitor by 180°. Hold the blood input gap (at the tip of the test strip) to the drops of blood until the gap is completely filled and the monitor in the display starts counting backwards.

Do not press the penetration area to the test strip. The blood must not be spread. The blood is sucked into the gap.

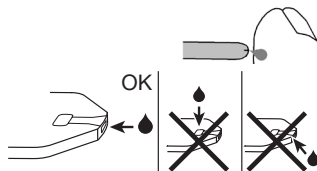

##### Note

Error message "Error 2" appears on the display if the gap was not correctly and sufficiently filled with blood. Repeat the measurement using a new test strip and a greater penetration depth.


## Note

- Do not apply blood to the sides of the test strips
- Do **not** add blood later if the device does not start measurement. Remove the test strip and end this test. Use a new test strip.
- If the test strip has already been inserted into the device but no blood is added to the test strip within two minutes, the device switches itself off. Briefly remove the test strip and reinsert it so that the device automatically switches itself back on.
- Contact Customer Services if you are unable to fill the test strip with blood correctly.

## 5.4 Reading the result and marking measurements

### Reading the result



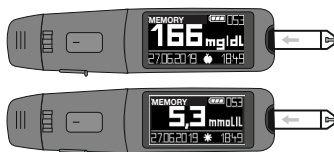

As soon as the blood input gap is filled with sufficient blood, the device performs the blood glucose measurement. The monitor counts down for approx. five seconds. The measurement is then shown on the display.



Read your measured value. Check again that you have read the result correctly. The underline must be below the measured value, otherwise you need to turn the monitor by 180°. For explanations of and measures regarding the measured values, see “5.6 Evaluating measured blood glucose values” on page 26. If an error message is displayed, read chapter “8. What if there are problems?” on page 34.

### Marking the measurement

You have the following options for marking measured values:

	No marking
	Before meal
	After meal
	General marking (e.g. after exercising).

Marking measured values enables you, your GP or diabetes consultant to better monitor your blood glucose values. For example, you can display the average values of all measurements taken before a meal.



To do this, proceed as follows:

- 1 Following the measurement, the display will briefly show the measured value and then the menu in which you can mark the measured value. It is not possible to change the marking afterwards.
- 2 Select the desired marking using the scroll wheel.
  - ○ "No marking"
  - ● "Before meal"
  - 🍷 "After meal"
  - \* "General marking"

• Confirm the marking by pressing the scroll wheel.
- 3 The selected marking is now allocated to the measured value and saved to the memory.


## 5.5 Post-processing and disposal

### 1 Remove test strip

Remove the test strip from the device and carefully dispose of it in accordance with the applicable regulations to avoid infecting others.

### 2 Remove the cap

Carefully remove the cap from the lancing device.



### 3 Stick protective disc on needle

Place the retained protective disc flat on a hard surface. Stick the tip of the needle into the protective disc (image 1) so the needle is covered (image 2).




Image 1





Image 2

#### 4 Remove and dispose of lancet needle

Press the trigger again so that you can grip the shaft. Carefully remove the lancet needle from the lancing device and dispose of the lancet in a puncture-proof container.

Carefully dispose of all blood samples and materials that came into contact with you or your patients. This prevents injuries and the infection of others.



#### 5 Replace cap

Place the cap back on the device.



### 5.6 Evaluating measured blood glucose values

Your blood glucose monitor can process measured values between 20 and 630 mg/dL (1.1 and 35.0 mmol/L). A warning message is displayed in the event of measured values lower than 20 mg/dL (1.1 mmol/L) and measured values higher than 630 mg/dL (35.0 mmol/L).



#### Warning

- If you suspect that the blood glucose results are incorrect, first repeat the test and, if necessary, perform a functional test using control solution. Seek medical advice if dubious results persist.
- Seek medical attention immediately if your symptoms do not correspond to your measured blood glucose values and you have followed all instructions for the Beurer GL50 evo blood glucose monitor.
- Do not ignore symptoms of too high/low blood glucose levels. Always seek medical attention!

#### Blood glucose values

The following tables list blood glucose values based on the STANDARDS OF MEDICAL CARE IN DIABETES 2016 from the ADA (American Diabetes Association).

Time of the blood glucose measurement	Normal blood glucose values	Increased risk of diabetes (prediabetes)*	Diabetes
On an empty stomach (fasting plasma glucose)	Below 100 mg/dL Below 5.6 mmol/L	100 – 125 mg/dL 5.6 – 6.9 mmol/L	≥ 126 mg/dL ≥ 7.0 mmol/L
Two hours after an oral glucose tolerance test (consumption of 75 g)	Below 140 mg/dL Below 7.8 mmol/L	140 – 199 mg/dL 7.8 – 11.0 mmol/L	≥ 200 mg/dL ≥ 11.1 mmol/L

\* The risk increases continually, beginning with values below the lower limit of the range and increasing disproportionately towards the upper limit of the range.





## Overview of glycaemic recommendations for non-pregnant adults with diabetes



A1C	< 7.0%* < 53 mmol/mol*
Preprandial capillary plasma glucose	80–130 mg/dL* 4.4–7.2 mmol/L*
Peak value of postprandial capillary plasma glucose**	< 180 mg/dL* 10.0 mmol/L*

\* For individual patients, more or less strict glycaemic targets may be appropriate. The target values should be adjusted depending on the length of time the person has had diabetes, age/life expectancy, accompanying diseases, known cardiovascular diseases or advanced microvascular complications, hypoglycaemia unawareness, as well as individual patient considerations.

\*\* The postprandial glucose value can serve as a target value if the A1C values are not met despite the preprandial glucose targets having been reached. Postprandial blood glucose measurements should be taken one to two hours after the start of a meal, as this is when diabetics' values are generally at the highest.

### Critical blood glucose values

Display	Blood glucose	Actions
	Very low blood glucose level  Below 20 mg/dL (below 1.1 mmol/L)	Immediately seek medical attention.
	Low blood glucose level  Below 70 mg/dL (below 3.9 mmol/L)	Have a suitable snack. Follow your GP's instructions.
	High blood glucose level  <ul style="list-style-type: none"> <li>On empty stomach, over 100 mg/dL (5.6 mmol/L)</li> <li>2 hours after a meal, over 140 mg/dL (7.8 mmol/L)</li> </ul>	If this high value persists 2 hours after your last meal, this may indicate hyperglycaemia (high blood glucose). Seek medical attention to coordinate any measures, if applicable.
	High blood glucose level, possibly ketones  Above 250 mg/dL (over 13.9 mmol/L)	Conduct ketone test For this purpose, seek medical attention.

Display		Blood glucose	Actions
		Very high blood glucose level  Above 630 mg/dL (over 35.0 mmol/L)	Take another measurement using a new test strip. If the display is the same as before: seek medical assistance immediately.

## 5.7 Functional check using control solution

The control solution is used to test the entire blood glucose monitoring system. This helps to determine whether the monitor and the test strips are working optimally together and whether the test is being performed correctly.

Perform the control solution test if you suspect that the blood glucose monitor and/or the test strips could be faulty or if you have repeatedly measured unusual blood glucose values. Also test the monitor if it has been dropped or is damaged. The control solution is available separately. For the control solution test, please observe the additional notes in the instructions for use for the control solution.

### Important

- Do not use third-party control solution. Correct functioning of your monitor can only be tested using Beurer LEVEL3 + LEVEL4 control solutions.
- Control solution measurements: when using the device, specialist personnel must follow statutory guidelines.
- Do not apply any blood samples or control solutions to the test strip before inserting it in the monitor.

### Performing a functional test using control solution

#### Warning


To obtain correct results, the measuring device, the test strip and the control solution must be the same temperature. For the “Functional test using the control solution”, the temperature is to be between 20°C and 26°C.

#### 1 Insert test strip

Hold the monitor so that the display is facing you. Insert a test strip into the slot on the monitor with the contacts first. Make sure that the front of the test strip is facing you (see section “3.5 Test strips”).

## 2 Activate control mode


Once you have inserted the test strip, the blood glucose monitor switches on automatically and briefly shows the initial display. Once the initial display has disappeared, quickly rotate the scroll wheel all the way from the left to the right until “CONTROL” appears at the top of the animation display.



**IMPORTANT:** Control solutions and blood react to temperature influences in different ways. It is therefore of vital importance that control solution measurement is always performed in control solution mode. If this mode is not used, results may be obtained that are outside the target range.

## 3 Drip control solution on surface

Choose a clean surface to carry out the functional test correctly. Shake the control solution well before use. Undo the cap and squeeze two drops next to each other on the clean surface without touching them. Use the second drop for the measurement.



### Note

Never apply the control solution straight from the bottle to a test strip. Reason: the remaining solution in the bottle will be contaminated if the top of the bottle comes into contact with the test strip.

## 4 Apply drop to the test strip

Hold the input gap (at the tip of the test strip) to the drop of control solution until the gap is completely filled. When the gap is sufficiently filled with solution, the device performs a measurement. The device counts down for approx. five seconds. The measurement is then shown on the display.

## 5 Evaluate result of functional test

Check whether the result is within the specified range of results for the control solution. This range of results is printed on the test strip box or the test strip packaging or on the information sheet included.

### Expected results

At room temperature, the measured values from the test using the control solution should be within the range printed on the test strip box in approx. 95% of all tests.



### Warning

The result range printed on the test strip box applies only to the control solution. **This is not a recommended value for your blood glucose level.**

If measurements are outside the specified range, check the following possible causes:

Cause	Action
<ul style="list-style-type: none"><li>• The first drop of control solution was not disposed of.</li><li>• The tip of the bottle was not cleaned correctly.</li><li>• The bottle was not shaken well enough.</li></ul>	Rectify the cause and repeat the test.
Control solution or test strip is contaminated.	Repeat the test using a new bottle of control solution and/or new test strip.
The control solution, test strip or blood glucose monitor is too warm or too cold.	Bring the control solution, test strip and monitor to room temperature (+20°C to +26°C) and repeat the test. The check performed at room temperature is used as a general functional check. The operating range specified in the technical specifications is valid without restriction.
The test strips and control solution were kept at a temperature and humidity outside the specified range.	Repeat the test using new, correctly stored accessories (test strips and control solution).
Damaged test strips. Possible causes include <ul style="list-style-type: none"><li>• Test strips were exposed to fresh air for too long.</li><li>• The test strip box was not closed completely.</li></ul>	Repeat the test using a new test strip and/or a new box of correctly stored test strips.
Test strip or control solution has expired.	Repeat the test using a new bottle of control solution and/or new test strip from a new box.
Functional test using control solution was performed incorrectly.	Repeat the test and follow the instructions.
Problem with the blood glucose monitor	Contact Customer Services.



### Warning

If you repeatedly obtain measured values outside the specified range when using control solution, **discontinue using the system to measure your blood glucose level.** Contact Customer Services.

## 6 MEASUREMENT MEMORY

For each measurement, your blood glucose value is automatically saved with the date and time unless “CL” was activated for a blood glucose measurement using control solution.

The memory can store a maximum of 480 measured values. If the memory is full, the oldest value is replaced by the most recent value. You can call up every individual measured blood glucose value. You can also calculate and display the average blood glucose value for the last 7, 14, 30 and 90 days.

## Note

- If you have already saved measured values and you reset the date, the average values are calculated as from the new period.
- “No saved values” indicates an empty memory for measured values. Press the ON/OFF button to switch off the device.

### 6.1 Displaying individual values

The most recent measured value is displayed first, and the oldest last. The date and time are also displayed on the monitor at the same time.

- 1 Switch on the blood glucose monitor by briefly pressing and holding the scroll wheel.
- 2 Rotate the scroll wheel until the arrow is pointing towards “All values”, then press the scroll wheel to confirm.




- 3 You can now rotate the scroll wheel to navigate between the saved individual values.
- 4 You can cancel the process at any time. To do so, press and hold the scroll wheel or wait until the device switches itself off automatically after 2 minutes.

### 6.2 Displaying average blood glucose values for marked values

You can display the average measured blood glucose value of the individual markings from the last 7, 14, 30 and 90 days.

- 1 Switch on the blood glucose monitor by briefly pressing and holding the scroll wheel.
- 2 Rotate the scroll wheel until the arrow is pointing towards “Average”, then press the scroll wheel to confirm.
- 3 Use the scroll wheel to select the desired marking (O, 🍏, 🍷 or ✨) for which you want to display the average values.




Ø 7 days	234 mg/dL	O
Ø 14 days	156 mg/dL	🍏
Ø 30 days	107 mg/dL	🍷
Ø 90 days	98 mg/dL	✨

Ø 7 days	13,0 mmol/L	O
Ø 14 days	8,7 mmol/L	🍏
Ø 30 days	5,9 mmol/L	🍷
Ø 90 days	5,4 mmol/L	✨

- 4 Press the scroll wheel to display the respective quantity of measured values in the markings.



7 days -	4 values	O
14 days -	10 values	🍏
30 days -	109 values	🍷
90 days -	407 values	✨

### 6.3 Evaluating measured values on a PC

The GL50 evo monitor features an integrated plug-in USB stick. The blood glucose evaluation software GlucoMemory is installed on the USB stick (for position of the USB connection, see page 11). The GL50 evo is compatible with Diabass and SiDiary.

The blood glucose evaluation software GlucoMemory is pre-installed on the monitor's USB stick. You can also install the software locally on a PC. This software enables you to evaluate your saved measured values, add insulin doses with manual entries and print or export your results as a PDF or CSV file. The software helps you and your GP to better monitor your blood glucose level.


For more information, please read software manual for the GlucoMemory software, including all the necessary information and a detailed description of how to use the software (in English and German language).

#### Note

- An effective evaluation is only possible if you have set the date and time correctly (see “Setting the date and time” on page 15).
- Measurements cannot be taken while the USB stick is connected to a PC.
- The measurements remain saved on the blood glucose monitor when the USB stick is removed from the PC.
- It is not possible to save software entries on the USB stick. Values are read only. If you want to make entries, please first install the software on your PC.

#### Evaluating measured values on the PC

- 1 The measuring device must be switched on. Insert the monitor's USB connector into a free USB port on your PC. In the event that the measuring device is not recognised, please try using another active USB port.
- 2 “USB” is shown on the display of the monitor. Saved data can now be viewed on your PC.
- 3 See the information on evaluating values in the software manual.



Alternatively, you can transfer the measured values to your smartphone/tablet using the optional Bluetooth® cap. The Beurer HealthManager app and software is available as a free download. For further information, please read the instructions for use included with the Bluetooth®-adapter.

## 7 STORING, MAINTAINING AND DISINFECTING THE DEVICE

### Storing

Keep the Beurer GL50 evo blood glucose monitor in the case supplied after each measurement and do not expose it to direct sunlight.



## Note

- Do not store the device, test strips and control solution in your vehicle, in the bathroom or in a cooling appliance.
- Retain these instructions for use.
- Only clean the device when it is switched off.
- The device needs to be in the location in which the measurement will be taken for at least 30 minutes before use so that the device can adapt to the ambient temperature. Please ensure that the operating range is between +10°C and +40°C. Accurate measurement results cannot be guaranteed if a measurement is taken outside of this temperature range.

## 7.1 Maintenance

Clean the surface of the device using a soft, slightly damp cloth (water or a mild cleaning solution). Dry the device using a lint-free cloth.

Make sure that moisture does not enter the test strip insertion slot. Do not spray cleaning products directly on the device. Do not submerge the device in water or any other fluids and make sure that no fluids can get into the device.

## 7.2 Disinfection

Please comply with the generally applicable guidelines on disinfection when using the device on different persons. Do not submerge the device in disinfection solutions or any other fluids and make sure that no fluids can enter the device.

The cap on the integrated lancing device can be disinfected with 70 – 75% alcohol. Disinfect the cap at least 1 x a week and submerge the cap in alcohol for approx. 10 minutes. Allow the cap to air dry.

## Note

The monitor is made of precision components. The accuracy of the measurements and service life of the device depend on its careful handling:

- Protect the device from impacts and do not drop it.
- Protect the device from damaging factors such as moisture, dirt, dust, blood, control solution or water, marked temperature fluctuations, direct sunlight and extreme cold.
- Do not use the device in the vicinity of strong electromagnetic fields, radio systems or mobile telephones.
- If the device is used in a dry environment, in particular near synthetic materials (clothes containing synthetic fibres and carpets, for example), the damaging static charges which occur may cause erroneous results.
- Do not use the device near sources of strong electromagnetic radiation, as this may affect normal operation.
- It is a good idea to carry out an assessment of the electromagnetic environment before using the device commercially.

## 8 WHAT IF THERE ARE PROBLEMS?

### Display messages on batteries and blood glucose measurement

No.	Cause	Solution
Empty battery	Batteries discharged.	Charge the blood glucose monitor via the USB interface.
High temperature	Temperature of the measuring environment, blood glucose monitor or test strip above the permitted range.	Repeat the test using a new test strip as soon as the measuring environment, monitor and test strip have reached room temperature (+20°C to +26°C). The check performed at room temperature is used as a general functional check. The operating range specified in the technical specifications is valid without restriction.
Low temperature	Temperature of the measuring environment, blood glucose monitor or test strip below the permitted range.	Repeat the test using a new test strip as soon as the measuring environment, monitor and test strip have reached room temperature (+20°C to +26°C). The check performed at room temperature is used as a general functional check. The operating range specified in the technical specifications is valid without restriction.
Strip error	Used or contaminated test strip inserted.	Insert an unused test strip that has not expired. Repeat the blood glucose measurement.
Error 1	System error.	Contact Customer Services.
Error 2	Insufficient amount of blood on the test strip.	Repeat the measurement using a new test strip.
Error 5	System error.	Contact Customer Services.
	Unknown error messages.	Contact Customer Services.

**Problem: device does not switch on**

Cause	Solution
ON/OFF switch set to off.	Move the ON/OFF switch to the right.
Battery dead.	Charge the blood glucose monitor via the USB port on a computer.
Test strip inserted incorrectly or not completely.	Firmly insert the test strip into the slot on the device with the contacts first. Make sure that the front of the test strip is facing you (see "Test strips" on page 13).
Device faulty.	Contact Customer Services.

**Problem: the test does not start after inserting the test strip into the device and applying blood**

Cause	Solution
Insufficient blood or test strip not filled correctly.	Repeat test using a new test strip and a larger drop of blood.
Faulty test strip.	Repeat the test using a new test strip.
Blood was applied while the device was switched off.	Repeat the test using a new test strip.
The basic settings of the device have been changed and these changes were not completed (see "4.2 Making and changing basic settings" on page 15).	Remove test strips and press and hold the scroll wheel until the device is switched off.
Device faulty.	Contact Customer Services.

## 9 TECHNICAL SPECIFICATIONS

<b>Dimensions (L x W x H)</b>	123 x 29 x 16 mm
<b>Weight</b>	36 g
<b>Power supply</b>	Li-ion rechargeable battery, 160 mAh
<b>Battery life</b>	150 measurements with fully charged rechargeable battery
<b>Measured value memory</b>	480 measured values with date/time Data retained when batteries are changed
<b>Average values</b>	For 7, 14, 30, 90 days
<b>Automatic switch-off</b>	2 minutes after last actuation
<b>Storage/transport temperature</b>	Temperature +2°C – +30°C Relative humidity: < 90%
<b>Operating ranges</b>	Temperature +10°C – +40°C Relative humidity: < 90% non-condensing
<b>Measurement range, glucose</b>	Glucose: 20–630 mg/dL (1.1 - 35.0 mmol/L)
<b>Blood sample</b>	Capillary whole blood, venous whole blood
<b>Required volume of blood</b>	0.6 microlitres
<b>Blood glucose measurement duration</b>	Approx. 5 seconds
<b>Calibration</b>	Plasma
<b>Testing method</b>	Amperometric bio sensor
<b>Usage</b>	Suitable for self-testing
<b>System function test</b>	Each time device is switched on

The serial number is located on the device or in the battery compartment.

### EMC

This device complies with the European standard EN 61326 and is subject to specific precautions with regard to electromagnetic compatibility. Please note that portable and mobile HF communication systems may interfere with this device. For more details, please contact our Customer Services at the address indicated.

### Test strip functionality

Test strips enable a quantitative measurement of the glucose level in fresh whole blood (capillary or venous). When the gap for taking blood comes into contact with a drop of blood, it is automatically filled by simple capillary action. The blood is sucked into the absorbing gap on the test strip and the monitor measures the glucose level in the blood.

The test is based on the measurement of an electric current that is generated by the chemical reaction of the glucose with the enzyme glucose dehydrogenase (*Aspergillus oryzae*) on the strip.

During the reaction, a mediator transports electrons through the electrode surface and so generates a current.

The monitor analyses this current. The current flow is proportional to the glucose content in the blood sample. The results are shown on the blood glucose monitor display. Only a small amount of blood is required (0.6 microlitres) and measurement takes approx. 5 seconds. The test strip detects blood glucose values from 20 to 630 mg/dL.

#### **Chemical components of the test strip sensor**

- FAD glucose dehydrogenase 6%
- Potassium ferricyanide 56%
- Non-reactive components 38%

#### **Control solution functionality**

The control solution contains a fixed amount of glucose that reacts with the test strip. A test with control solution is similar to a blood test. However, control solution is used instead of blood. The measurement using control solution must be within the result range. This range is printed on each test strip box.

#### **Chemical composition of the control solution**

The control solution is a red solution with the following D-glucose level (in percentage shares).

Substances	LEVEL 3 control solution	LEVEL 4 control solution
D-glucose	0.14%	0.37%
Non-reactive components	99.86%	99.63%

#### **Standards**

The Beurer GL50 evo blood glucose monitor complies with the European standards: IVD (98/79/EEC) and MDD (93/42/EEC).

## **10 COMPARISON OF MEASURED VALUES WITH LABORATORY VALUES**

#### **Precision**

Three lots of the GL50 evo blood glucose test strips have been tested to assess the precision of the GL50 evo blood glucose monitoring system. This includes a repeat assessment using venous blood and a laboratory precision assessment using the control material. The blood glucose content of the venous blood samples ranges from 42.7 to 418.0 mg/dL (2.37 to 23.20 mmol/L) and control material from three concentrations is used.

## Results of the repeat precision measurements

Sample	Venous blood		Overall average value		Pooled standard deviation		Pooled coefficient of variation (%)
	mg/dL	mmol/L	mg/dL	mmol/L	mg/dL	mmol/L	
1	42.7	2.4	36.0	2.0	2.0	0.1	5.6
2	62.0	3.4	59.2	3.3	3.5	0.2	5.9
3	120.5	6.7	127.1	7.1	4.1	0.2	3.2
4	201.0	11.2	213.8	11.9	6.7	0.4	3.1
5	316.5	17.6	329.9	18.3	10.1	0.6	3.1
6	418.0	23.2	433.5	24.1	14.5	0.8	3.3

## Results of the intermediate precision measurement

Sample	Control material		Overall average value		Pooled standard deviation		Pooled coefficient of variation (%)
	mg/dL	mmol/L	mg/dL	mmol/L	mg/dL	mmol/L	
1	70.0	3.9	71.3	4.0	1.0	0.1	1.4
2	135.6	7.5	136.3	7.6	1.4	0.1	1.1
3	351.5	19.5	350.8	19.5	2.8	0.2	0.8

## System accuracy

The GL50 evo blood glucose monitor in comparison to the YSI.

Three lots of GL50 evo blood glucose test strips have been tested to assess the system accuracy of the GL50 evo blood glucose monitoring system and to compare it with the reference method, in which capillary whole blood concentrations of 36.0 mg/dL (2.0 mmol/L) to 442.5 mg/dL (24.6 mmol/L) have been used.

## Results of the system accuracy for glucose concentrations <100 mg/dL (<5.55 mmol/L)

Within $\pm 5$ mg/dL (Within $\pm 0.28$ mmol/L)	Within $\pm 10$ mg/dL (Within $\pm 0.56$ mmol/L)	Within $\pm 15$ mg/dL (Within $\pm 0.83$ mmol/L)
101/168 (60.12%)	161/168 (95.83%)	166/168 (98.81%)

## Results of the system accuracy for glucose concentrations $\geq 100$ mg/dL ( $\geq 5.55$ mmol/L)

Within $\pm 5\%$	Within $\pm 10\%$	Within $\pm 15\%$
182/432 (42.13%)	358/432 (82.87%)	426/432 (98.61%)

## Results of the system accuracy for combined glucose concentrations between 36.0 mg/dL (2.0 mmol/L) and 442.5 mg/dL (24.6 mmol/L).

Within  $\pm 15$  mg/dL or  $\pm 15\%$   
(within  $\pm 0.83$  mmol/L or  $\pm 15\%$ )

592/600 (98.67%)

In comparison to the YSI, the GL50 evo met the EN ISO 15197:2015 standard, whereby 95% of the blood glucose values measured have to fall within the following zones: either  $\pm 15$  mg/dL ( $\pm 0.83$  mmol/L) of the measured average values when using the reference measuring procedure for blood glucose concentrations  $< 100$  mg/dL ( $< 5.55$  mmol/L) or  $\pm 15\%$  for blood glucose concentrations of  $\geq 100$  mg/dL ( $\geq 5.55$  mmol/L). 99% of the individual measured blood glucose values must fall within zones A and B of the Consensus Error Grid (CEG) for diabetes type 1.

### Performance evaluation by the user

A study to assess the glucose values of blood samples of capillary blood from the fingertips, which were obtained from 103 individuals that had no special training, produced the following results: 96.7% within  $\pm 15$  mg/dL ( $\pm 0.83$  mmol/L) and 95.9% within  $\pm 15\%$  of the values obtained in the medical laboratory with glucose concentrations of at least 100 mg/dL (5.55 mmol/L).

You will find further details and information regarding blood glucose results and various technologies in generally relevant specialist medical literature.

## 11 USAGE LIMITS FOR SPECIALIST PERSONNEL FROM THE HEALTHCARE SECTOR

1. If the patient exhibits the following symptoms, it may be the case that no correct values can be obtained:
  - Acute dehydration
  - Acute hypotension (low blood pressure)
  - Shock
  - Hyperosmolar hyperglycaemic condition (with or without ketosis)
2. Lipaemic samples: cholesterol levels up to 500 mg/dL (13 mmol/L) and triglyceride levels up to 1000 mg/dL (11.4 mmol/L) do not influence the results. Severely lipaemic blood samples were not tested with the Beurer GL50 evo blood glucose monitoring system; therefore, using the device with these samples is not recommended.
3. In the case of severely ill patients, blood glucose monitors for home use should not be used.
4. The effect of interfering substances on the measurements depends on the concentration in the blood. The maximum concentrations of certain substances listed below do not significantly influence the measurements.

Concentration of tested substances	Influence	Blood glucose value	50-100 mg/dL (2.8-5.6 mmol/L)	250-350 mg/dL (13.9-19.4 mmol/L)
Acetaminophen	7 mg/dL	(0.46 mmol/L)	6.6 mg/dL (0.37 mmol/L)	4.5%
Ascorbic acid	4 mg/dL	(0.23 mmol/L)	3.3 mg/dL (0.18 mmol/L)	5.1%
Bilirubin	3.3 mg/dL	(0.06 mmol/L)	0.1 mg/dL (0.01 mmol/L)	-1.4%
Cholesterol	400 mg/dL	(10.34 mmol/L)	-6.8 mg/dL (-0.38 mmol/L)	-6.2%
Creatinine	30 mg/dL	(2.65 mmol/L)	0.0 mg/dL (0.00 mmol/L)	-0.1%
Dopamine	2.2 mg/dL	(0.14 mmol/L)	5.0 mg/dL (0.28 mmol/L)	1.0%
EDTA	5.0 mg/dL	(0.17 mmol/L)	-2.0 mg/dL (-0.11 mmol/L)	-2.4%
Ephedrine	40 mg/dL	(2.42 mmol/L)	-3.9 mg/dL (-0.22 mmol/L)	2.4%
Galactose	20 mg/dL	(1.11 mmol/L)	-3.1 mg/dL (-0.17 mmol/L)	0.5%
Gentisic acid	7 mg/dL	(0.45 mmol/L)	7.2 mg/dL (0.40 mmol/L)	2.9%
Glutathione	1 mg/dL	(0.03 mmol/L)	-2.6 mg/dL (-0.14 mmol/L)	-3.7%
Haemoglobin	300 mg/dL	(0.05 mmol/L)	-3.1 mg/dL (-0.17 mmol/L)	-2.6%
Heparin	2.1 mg/dL	(0.0018 mmol/L)	-3.0 mg/dL (-0.17 mmol/L)	-1.3%
Ibuprofen	50 mg/dL	(2.43 mmol/L)	-2.6 mg/dL (-0.15 mmol/L)	-1.9%
Icodextrin	1094 mg/dL	(0.64-0.78 mmol/L)	-4.17 mg/dL (-0.23 mmol/L)	-2.9%



Concentration of tested substances	Influence	Blood glucose value	50-100 mg/dL (2.8-5.6 mmol/L)	250-350 mg/dL (13.9-19.4 mmol/L)
L-Dopa	2 mg/dL	(0.10 mmol/L)	9.3 mg/dL (0.52 mmol/L)	7.9%
Maltose	278 mg/dL	(7.72 mmol/L)	-1.53 mg/dL (-0.09 mmol/L)	-2.6%
Methyldopa	4 mg/dL	(0.19 mmol/L)	7.3 mg/dL (0.41 mmol/L)	0.9%
Pralidoxime iodide	5 mg/dL	(0.14 mmol/L)	1.7 mg/dL (0.09 mmol/L)	-0.1%
Sodium salicylate	40 mg/dL	(2.50 mmol/L)	-3.1 mg/dL (-0.17 mmol/L)	-0.6%
Salicylic acid	60 mg/dL	(4.34 mmol/L)	-0.1 mg/dL (-0.01 mmol/L)	7.6%
Tolbutamide	100 mg/dL	(3.70 mmol/L)	0.5 mg/dL (0.03 mmol/L)	-0.8%
Tolazamide	2.5 mg/dL	(0.08 mmol/L)	-2.3 mg/dL (-0.13 mmol/L)	1.8%
Triglyceride	800 mg/dL	(9.37 mmol/L)	-7.50 mg/dL (-0.42 mmol/L)	-4.0%
Uric acid	16.5 mg/dL	(0.98 mmol/L)	6.6 mg/dL (0.37 mmol/L)	1.8%
Xylose	9.5 mg/dL	(0.63 mmol/L)	5.6 mg/dL (0.31 mmol/L)	6.6%

## 12 WARRANTY/SERVICE

Beurer GmbH, Söflinger Straße 218, 89077 Ulm, Germany (hereinafter referred to as “Beurer”) provides a warranty for this product, subject to the requirements below and to the extent described as follows.

**The warranty conditions below shall not affect the seller’s statutory warranty obligations which ensue from the sales agreement with the buyer.**

**The warranty shall apply without prejudice to any mandatory statutory provisions on liability.**

Beurer guarantees the perfect functionality and completeness of this product.

The worldwide warranty period is 5 years, commencing from the purchase of the new, unused product from the seller.

The warranty only applies to products purchased by the buyer as a consumer and used exclusively for personal purposes in the context of domestic use.  
German law shall apply.

During the warranty period, should this product prove to be incomplete or defective in functionality in accordance with the following provisions, Beurer shall carry out a repair or a replacement delivery free of charge, in accordance with these warranty conditions.

**If the buyer wishes to make a warranty claim, they should approach their local retailer in the first instance: see the attached “International Service” list of service addresses.**

The buyer will then receive further information about the processing of the warranty claim, e.g. where they can send the product and what documentation is required.

A warranty claim shall only be considered if the buyer can provide Beurer, or an authorised Beurer partner, with

- a copy of the invoice/purchase receipt, and
- the original product.

The following are explicitly excluded from this warranty:

- deterioration due to normal use or consumption of the product;
- accessories supplied with this product which are worn out or used up through pro per use (e.g. batteries, rechargeable batteries, cuffs, seals, electrodes, light sources, attachments and nebuliser accessories);
- products that are used, cleaned, stored or maintained improperly and/or contrary to the provisions of the instructions for use, as well as products that have been opened, repaired or modified by the buyer or by a service centre not authorised by Beurer;
- damage that arises during transport between manufacturer and customer, or between service centre and customer;
- products purchased as seconds or as used goods;
- consequential damage arising from a fault in this product (however, in this case, claims may exist arising from product liability or other compulsory statutory liability provisions).

Repairs or an exchange in full do not extend the warranty period under any circumstances.





GL 50 evo

Beurer GmbH • Söflinger Straße 218 • 89077 Ulm, Germany  
www.beurer.com • www.beurer-healthguide.com



SteriLance Medical (Suzhou) Inc.  
No. 168, PuTuoShan Road,  
New District, Suzhou 215153, China



Emergo Europe  
Prinsessegracht 20,  
2514 AP The Hague,  
The Netherlands

